RISHABH

Data Sheet

RISH Multi 12S...18S

Analog - Digital multimeters

RoHS CE

Measure Control Record Analyze Optimize

Application

It is Analog Digital Multimeter which measures VAC, VDC, VAC+DC,Frequency, mA DC, mA (AC+DC), Resistance, continuity, Diode, Farad, AC current measurement.

Product Features

Automatic Terminal Blocking System (ABS)
The automatic Terminal blocking system prevents incorrect connection of the test leads and incorrect selection of the measured quantity. This reduces danger to the user, the meter and the system to a remarkable extent.

Interface And Software RISH com 100
The multimeters are fitted with a serial RS-232 C interface via which the measured values can be transmitted to a PC. These values, electrically isolated, are transmitted to the attachable interface adaptor with infrared light through the case*

MIN/MAX Value Storage
In addition to the display of the actual measured value, the minimum or maximum value can constantly be updated and stored.

Indication Of Negative Values On The Analog Scale
When measuring DC quantities, also negative values are shown on the analog scale so that variations of the measured value can be observed at the zero point.

Indication Of Negative Values On The Analog Scale
The measuring principle employed permits the measurement of the root-mean-square value (TRMS) of AC quantities and mixed quantities (AC and DC) regardless of the waveform.

Automatic Data Hold*
The DATA HOLD function makes it possible to hold the digitally displayed measured value. According to a patented method, it is ensured that no freak value but the actual measured value is held in the case of rapid changes in measured quantities. The held measured value appears on the digital display. The actual measured value continues to be shown on the analog scale.

Autoranging / Manual Range Selection
The measured values are selected with rotary switch.
The measuring range is automatically matched to the measured value. The measuring range can also be selected manually via the AUTO/MAN push button.

Continuity Test
This permits testing for short circuit and open circuit. In addition to the display, a facility of sound signal is available.

Temperature Measurement
It is possible to use all models of RISH *multi* series, in direct connection of temperature sensor Pt 100 / Pt 1000. The meters automatically detects the type of sensors connected to it & displays directly measured temperature.

Signalling in the case of a blown fuse
The display FUSE points to a blown fuse.

Power economizing circuit
The meter disconnects automatically when the measured value remains unchanged for about 10 minutes and no operating control was operated during this time. The disconnection facility can be disabled.

Overload Warning
A sound signal indication violation of the overload limits.

Protective holster for rough duty
A holster of soft rubber with tilt stand protects the meter against damage in the case of shock and drop. The rubber material makes for the meter to stand firmly even on vibrating surface.

Top model *RISH* multi 18S
The top model Rish multi 18S features a 4 3/4 digit display (31 000 digits)as well as the following additional functions : Event counter, measurement of the duration of the event, time counter (stop watch), data compare,dB measurment, wide-range capacitance measurement.

Calibration
RISH multi is automatically calibrated with respect to Fluke 5500 / Wavetek 9100. Automatic calibration is done through a developed calibration software with RS232 connection to the multimeter. Every multimeter is provided with the Test Certificate which is traceable to National / International standards. All the meters can be recalibrated at the Rishabh Instruments.

* Protected by patent rights

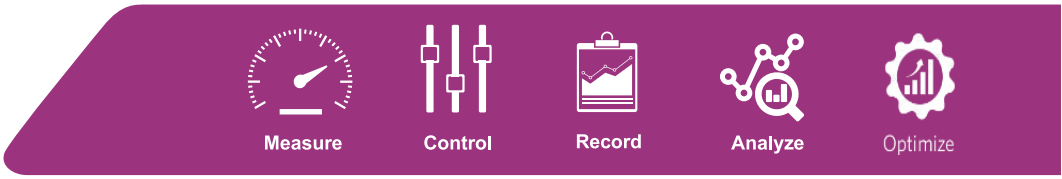

Specifications RISH *multi* 12S... 16S

Meas. function	Measuring range	12S	13S	14S	15S	16S	Resolution	Input impedance	Inherent deviation of the digital display ± (...% of meas. val. + ...digits) for reference condition 12S	13S	14S	15S	16S	4) Overload capacity: Overload value	Overload duration	Measuring function
	RISH*Multi*															
V⎓	30.00 mV	●	●	●	●	●	10 µV	> 10G Ω // < 40 pF	0.5 +3 5)				0.5 + 3 5)	1000 V DC AC effective sinusoidal	cont.	V⎓
	300.0mV	●	●	●	●	●	100 µV	> 10G Ω// < 40 pF	0.5 + 3				0.5 + 3			
	3.000 V	●	●	●	●	●	1 mV	11M Ω // < 40 pF	0.25 +1				0.1 + 1			
	30.00 V	●	●	●	●	●	10 mV	10M Ω // < 40 pF	0.25 + 1				0.1 + 1			
	300.0 V	●	●	●	●	●	100 mV	10M Ω // < 40 pF	0.25 + 1				0.1 + 1			
	1000 V	●	●	●	●	●	1 V	10M Ω// < 40 pF	0.35 + 1				0.1 + 1			
V~	3.000 V	●	●	●	●	●1)	1 mV	11M Ω // < 40 pF	0.75 + 2(10... 300 D) 0.75 + 1 (> 300 D)				0.75 + 3 (> 10 D)			V~
	30.0 V	●	●	●	●	●1)	10 mV	10M Ω // < 40 pF								
	300.0 V	●	●	●	●	●1)	100 mV	10M Ω // < 40 pF								
	1000 V	●	●	●	●	●1)	1 V	10M Ω // < 40 pF								
V⎓~	3.000 V					●1)	1 mV	11M Ω // < 40 pF	—	—	—	—	0.75 + 3 (> 10 D)			V⎓~
	30.00 V					●1)	10 mV	10M Ω // < 40 pF	—	—	—	—				
	300.0 V					●1)	100 mV	10M Ω // < 40 pF	—	—	—	—				
	1000 V					●1)	1 V	10M Ω // < 40 pF	—	—	—	—				
								Voltage drop. approx. 12S / 13S / 14S / 15S/16S								
A⎓	300.0 µA			●	●	●	100 nA	— / --- / 15 mV	---	---	1.0 + 5 (> 10D)		0.5 + 5 (> 10 D)	0.36 A	cont.	A⎓
	3.000 mA	●	●	●	●	●	1 µA	15 mV / 15 mV / 150 mV	1.0 + 5 (> 10D)		1.0 + 2		0.5 + 2			
	30.00 mA	●	●	●	●	●	10 µA	150 mV / 150 mV / 650 mV	0.25 + 2		1.0 + 5 (<10 D)		0.5 + 5 (> 10 D)			
	300.0 mA	●	●	●	●	●	100 µA	1 V / 1 V / 1 V	1.0 + 2				0.5 + 2			
	3.000 A		●	●	●	●	1 mA	--- / 100 mV / 100 mV	--	1.0 + 5 (> 10 D)			1,0 + 5 (> 10 D)	7)	7)	
	10.00 A		16A	●	●	●	10 mA	--- / 300/270mV / 270 mV	---	1.0 + 2			1,0 + 2			
A~	3.000 mA			●	●		1 µA	--- / --- / 150 mV	--	---	1.5 + 2 (> 10 D)		--	0.36 A	cont.	A~
	30.00 mA	●	●				10 µA	150 mV / 150 mV / —	1.5 + 2 (> 10 D)		---	---	--			
	300.0 mA	●	●	●	●		100 µA	1 V / 1 V / 1 V	1.5 + 2 (> 10D)				--	7)	7)	
	10.00 A		16A	●	●		10 mA	--- / 300/270mV / 270 mV	---	1.5 + 2 (> 10 D)			--			
A~	30.00 A 2)	●					10 mA	150 mV / --- / —	1.5 + 2 (> 10 D)	---	---	--	--	0.36 A	cont.	A~
	300.0 A 2)	●					100 mA	1 V / --- / --	---	---	---	--	--			
A⎓~	3.000 mA					●1)	1 µA	--- / --- / 150 mV	---	---	---	--	1.5 + 4 (> 10 D)	12 A	10 min	A⎓~
	300.0 mA					●1)	100 µA	--- / --- / 1 V	--	---	---	--	1.5 + 4 (> 10 D)			
	10.00 A					●1)	10 mA	--- / --- / 270 mV	---	---	---	--	1,75 + 4 (> 10 D)			
								No-load voltage								
Ω	30.00 Ω	●	●	●	●	●	10 m Ω	max. 3.2 V	0.5 + 3 5)				0.4 + 3 5)	1000 V DC AC effective sinusoidal	10 min	Ω
	300.0 Ω	●	●	●	●	●	100 m Ω	max. 3.2 V	0.5 + 3				0.4 + 3			
	3.000 k Ω	●	●	●	●	●	1 Ω	max. 1.25 V	0.4 + 1				0.2 + 1			
	30.00 k Ω	●	●	●	●	●	10 Ω	max. 1.25 V	0.4 + 1				0.2 + 1			
	300.0 k Ω	●	●	●	●	●	100 Ω	max. 1.25 V	0.4 + 1				0.2 + 1			
	3.000 M Ω	●	●	●	●	●	1 k Ω	max. 1.25 V	0.6 + 1				0.4 + 1			
	30.00 M Ω	●	●	●	●	●	10 k Ω	max. 1.25 V	2.0 + 1				2.0 + 1			
→|←	2.000 V	●	●	●	●	●	1 mV	max. 3.2 V	0.25 + 1				0.1 + 1			→|←
								Discharge resistance / $U_{0\ max}$								
F	30.00 nF				●	●	10 pF	250 k Ω / 2.5 V	—	---	—	1.0 + 3 6)		1000 V DC / AC effective sinusoidal	10 min	F
	300.0 nF				●	●	100 pF	250 k Ω / 2.5 V	—	---	—	1.0 + 3				
	3.000 µF				●	●	1 nF	25 k Ω / 2.5 V	—	---	—	1.0 + 3				
	30.00 µF				●	●	10 nF	25 k Ω / 2.5 V	—	---	—	3.0 + 3				
								Sensor / F_{min} V ⎓ / F_{min} V ~								
Hz	300.0 Hz				●	●	0.1 Hz	1 Hz / 45 Hz	—	---	—	0.5 + 1 8)		≤ 3 kHz: 1000V ≤ 30 kHz: 300V ≤100 kHz: 30 V	cont.	Hz
	3.000 kHz				●	●	1 Hz	1 Hz / 45 Hz	—	---	—					
	30.00 kHz				●	●	10 Hz	10 Hz / 45 Hz	—	---	—					
	100.0 kHz				●	●	100 Hz	100 Hz / 100 Hz	—	---	—					
%	2.0... 98.0 %				●	●	0.1 %	1 Hz / --	---	---	—	1 Hz.....1kHz: ± 5 D 9) 1Hz.....10kHz:±5 D/kHz 9)				%
°C	- 200.0... + 200.0°C	●	●	●	●	●	0.1°C	Pt 100 / --- / --	2 Kelvin + 5 D 10)					1000 V DC AC effective sinusoidal	10 min	°C
	+ 200.0... + 850.0°C	●	●	●	●	●	0.1°C		1.0 + 5 10)							
	-100.0... + 200.0°C	●	●	●	●	●	0.1°C	Pt 1000 / --- / --	2 Kelvin + 2 D 10)							
	+ 200.0 ... + 850.0°C	●	●	●	●	●	0.1°C		1.0 + 2 10)							

1) TRMS measurement
2) Direct display with clip-on transformer 1000:1
4) At 0°C... + 40°C
5) With zero setting; w/o zero setting + 35 digits
6) With zero setting; w/o zero setting + 50 digits
7) RISH multi 13S (w/o 16 A fuse!) : 16A cont., 20A for 5 min; RISH multi 14S... 16S: 12A for 5 min, 16A for 30s

8) Range 3 V ⎓~ U_E = 1.5 V_{rms} ... 100 V_{rms}
30 V ⎓~ U_E = 15 V_{rms} ... 300V_{rms}
300 V ⎓~ U_E = 150 V_{rms} ... 1000V_{rms}

9) On the range 3V⎓ rectangular signal positive at one end 5 ... 15 V, f = const., not 163.84 Hz or integer multiple.
10) Without sensor

Specifications RISH *multi* 18S

Meas. function	Measuring range	Resolution	Input impedence		Inherent error of the digital display ± (...% of rdg.+... digits) at reference conditions		2) Overload capacity		Meas. function
			⎓	~ 1) ⎓ 1)	⎓	~ 1) ⎓ 1)	Overload value	Overload duration	
V	300.00 mV	10 µV	>10 G Ω	5 MΩ// < 40 pF	0.05 + 3; 0.05 + 20 3)	1.0 + 30 (> 600 Digit)	1000 V DC AC RMS sinusoidal	cont.	V
	3.0000 V	100 µV	11 M Ω	5 MΩ// < 40 pF	0.05 + 3	0.5 + 30 (> 300 Digit)			
	30.000 V	1 mV	10 M Ω	5 MΩ// < 40 pF	0.05 + 3	0.5 + 30 (> 300 Digit)			
	300.00 V	10 mV	10 M Ω	5 MΩ// < 40 pF	0.05 + 3	0.5 + 30 (> 300 Digit)			
	1000.0 V	100 mV	10 M Ω	5 MΩ// < 40 pF	0.05 + 3	0.5 + 30 (> 300 Digit)			
dB	See table below		—	as at V~	—	± 0.5 dB 4)			dB
			Voltage drop. approx.						
			⎓	~ 1) ⎓ 1)	⎓	~ 1) ⎓ 1)			
mA	300.00 µA	10 nA	15 mV	15 mV	0.2 + 20	1.2 + 30 (> 300 Digit)	0.36 A	cont.	mA
	3.0000 mA	100 nA	150 mV	150 mV	0.2 + 10	1.2 + 30 (> 300 Digit)			
	30.000 mA	1 µA	30 mV	30 mV	0.05 + 10	1.2 + 50 (> 300 Digit)			
	300.00 mA	10 µA	300 mV	300 mV	0.2 + 10	1.2 + 30 (> 300 Digit)			
A	3.0000 A	100 µA	150 mV	150 mV	0.5 + 10	1.2 + 50 (> 300 Digit)	12A 5)	5 min	A
	10.000 A	1 mA	400 mV	400 mV	0.5 + 10	1.2 + 30 (> 300 Digit)			
			No-load voltage	Short circuit current					
Ω	300.00 Ω	10 m Ω	max. 4.00 V	max. 1 mA	0.1 + 6; 0.1 + 30 3)		1000 V DC AC RMS sinusoidal	1 min	Ω
	3.0000 k Ω	100 m Ω	max. 1.25 V	max. 100 µA	0.1 + 6				
	30.000 k Ω	1 Ω	max. 1.25 V	max. 10 µA	0.1 + 6				
	300.00 k Ω	10 Ω	max. 1.25 V	max. 1 µA	0.1 + 6				
	3.0000 M Ω	100 Ω	max. 1.25 V	max. 0.1 µA	0.1 + 6				
	30.000 M Ω	1k Ω	max. 1.25 V	max. 0.1 µA	1.0 + 6				
⊣▶	3.0000 V-	1mV	max. 4.00 V	—	0.2 + 3				⊣▶
			Discharge resist.	U_{0max}					
F	3.000 nF	1 pF	1.5 M Ω	4 V	1.0 + 8; 1.0 + 60 3)		1000 V DC AC RMS sinusoidal	1 min	F
	30.00 nF	10 pF	1.5 M Ω	4 V	1.0 + 8; 1.0 + 30 3)				
	300.0 nF	100 pF	150 k Ω	4 V	1.0 + 3				
	3.000 µF	1 nF	150 k Ω	4 V	1.0 + 3				
	30.00 µF	10 nF	15 k Ω	2 V	1.0 + 3				
	300.0 µF	100 nF	1.5 k Ω	2 V	5.0 + 6				
	3000 µF	1 µF	1.5 k Ω	2 V	5.0 + 6				
	10000 µF	10 µF	1.5 k Ω	2 V	5.0 + 6				
			f_{min} 6)						
Hz	300.00 Hz	0.01 Hz	10 Hz		0.1 + 3 7)		≤ 3 kHz; 1000 V ≤ 30 kHz; 300 V ≤ 100 kHz 30 V	cont.	Hz
	3.0000 kHz	0.1 Hz	10 Hz						
	30.000 kHz	1 Hz	10 Hz						
	100.00 kHz	10 Hz	100 Hz						
°C	Pt 100 - 200.0... + 100.0 °C	0.1 °C	—	—	0.5 Kelvin + 3 8)		1000 V DC AC rms sine	1 min.	°C
	Pt 100 + 100.0... + 850.0 °C	0.1 °C	—	—	0.5 + 3 8)				
	Pt 1000 - 100.0... + 100.0 °C	0.1 °C	—	—	0.5 Kelvin + 3 8)				
	Pt 1000 + 100.0... + 850.0 °C	0.1 °C	—	—	0.5 + 3 8)				

dB ranges

Measuring ranges	Display span at reference voltage U = 0.775 V	Display span at reference voltage U_{ref} (V)
300 mV ~	- 48 dB... - 8 dB	- 40 dB... + 110 dB
3 V~	- 38 dB... + 12 dB	-60 dB... + 100 dB
30 V~	- 18 dB... + 32 dB	- 80 dB... + 80 dB
300 V~	+ 2dB... + 52 dB	- 100 dB... + 60 dB
1000 V~	+ 22 dB... + 63 dB	- 110 dB... + 40 dB
	Display (dB) = 20 lg U_x(V) / 0.775 V	Display (dB) = 20 lg U_x(V) / U_{ref} (V)

1) TRMS measurement
values < 100 digit (<500 digit for measuring range 300mV) will be supressed
2) At - 10 °C... + 40 °C
3) With zero adjuster; without zero adjuster
4) At a resolution of 0.01 dB
5) 16 A for 30s
6) Lowest measurable frequency with a sinusoidal measuring signal which is symmetrical to zero
7) Range 3 V ⎓: U_e = $1V_{eff/rms}$ ... $10 V_{eff/rms}$
30 V ⎓: U_e = $10V_{eff/rms}$ ... $100 V_{eff/rms}$
300 V ⎓: U_e = $100V_{eff/rms}$ ... $1000 V_{eff/rms}$
8) Without sensor

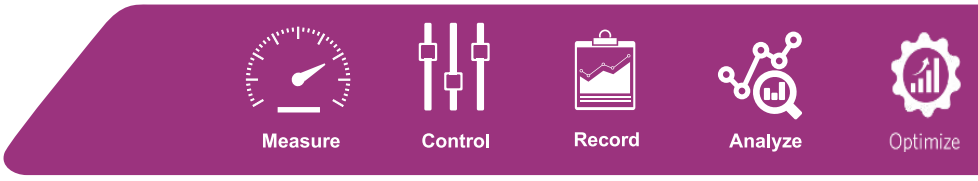

Reference conditions

Ambient temperature	+23Co + 2K
Relative humidity	45%... 55%
Frequency of the measured quantity	45 Hz... 65 Hz
Waveform of the measured quantity	Sinusoidal
Battery voltage	8V + 0.1 V

Measuring voltage with resistance measurement 12S ... 16S

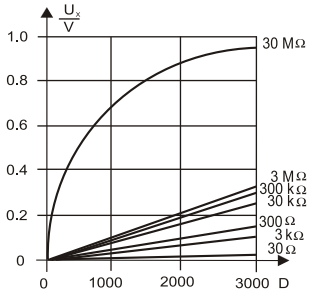

Voltage U_x across the resistance R_x to be measured as a function of measuring range and display.

Measuring voltage with resistance measurement 18S

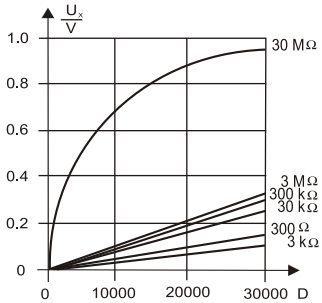

Voltage U_x across the resistance R_x to be measured as a function of measuring range and display.

Measuring current with diode test and / or continuity test 12S ... 16S

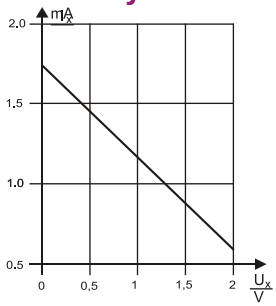

Measuring current I_x as a function of the displayed voltage U_x on the device under test.

Measuring current with diode test and / or continuity test 18S

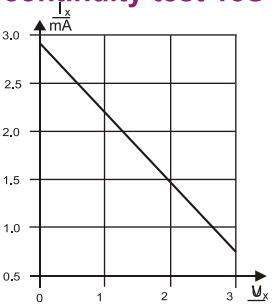

Measuring current I_x as a function of the displayed voltage U_x on the device under test.

Influence quantities and variations for 12S... 16S

Influence quantity	Influence range	Measured quantity / measuring range	Variation 1) ± (...% of meas. val. +... digits) 12S...	14S	15S	16S
Temperature	0 °C... + 21 °C and +25 °C... + 40 °C	30/300 mV ⎓	1.0 + 3			1.0 + 1
		3... 300 V ⎓	0.15 + 1			0.1 + 1
		1000 V ⎓	0.2 + 1			0.1 + 1
		V ~	0.4 + 2			0.3 + 2
		300 µ A 2) ... 300 mA ⎓	0.5 + 1			0.15 + 1
		3A / 10 (16) A ⎓	0.5 + 1			
		A ~	0.75 + 1			0.75 + 3
		30 Ω 2)	0.15 + 2			
		300 Ω	0.25 + 2			0.15 + 2
		3 kΩ... 3 M Ω	0.15 + 1			0.1 + 1
		30 M Ω	1.0 + 1			0.6 + 1
		30 nF 2) ... 3 µF	---			0.5 + 2
		30 µF	---			2.0 + 2
		Hz	---			0.5 + 1
		%	---			± 5 D
		-200... + 200 °C	0.5 K + 2			
		+ 200... + 850 °C	0.5 + 2			
Frequency of the measured quantity	15 Hz... < 30 Hz	3 ... 300 V ~	—		---	1.0 + 3
	30 Hz... < 45 Hz		—		---	0.5 + 3
	> 65 Hz... 400Hz		2.0 + 3			0.5 + 3
	> 400 Hz... 1 kHz		2.0 + 3			1.0 + 3
	> 1kHz... 20 kHz		---		---	2.0 + 3
	15 Hz... < 30 Hz	1000 V ~	—		---	1.0 + 3
	30 Hz... < 45 Hz		—		---	0.5 + 3
	> 65 Hz... 1kHz		3.0 + 3			2.0 + 3
	15 Hz... < 30 Hz	A~	---			1.0 + 3
	30 Hz... <45 Hz		---			0.5 + 3
	> 65 Hz... 1kHz		2.0 + 3			3.0 + 3
	Crest factor CF 1 ...3	V ~ 4), A~ 4)	—		---	± 1% of rdg.
	> 3 ...5		---		---	± 3 % of rdg.

The permissible crest factor CF of the AC quantity to be measured is a function of the displayed value :

Waveform of the measured quantity 3)

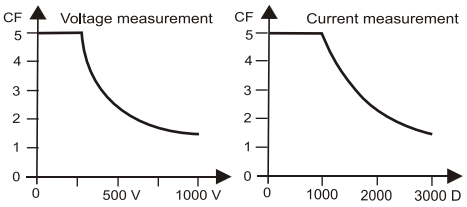

Influence quantity	Influence range	Measured quantity / measuring range	Variation 12S... 16S
Battery voltage	⊣⊢ 5) ... < 7.9 V > 8.1 V... 10.0 V	V ⎓	± 2 D
		V ~	± 4 D
		A ⎓	± 4 D
		A~	± 6 D
		30 Ω / 300 Ω/ °C	± 4 D
		3 kΩ... 30 M Ω	± 3 D
		nF, µF	± 1 D
		Hz	± 1 D
		%	± 1 D
Relative humidity	75 % 3 days Meter off	V ⎓ A ⎓ Ω F Hz %	1x Intrinsic error
DATA		°C	± 1 D
MIN / MAX		V ⎓, A ⎓	± 2 D

1 With temperature; Error data is per 10 K change in temperature. With frequency; Error data is valid from a display of 300 digits.
2 With zero setting
3 With unknown waveform (crest factor CF > 2), the measurement must be made with manual range selection.
4 Except for sinusoidal waveform
5 From the time the symbol "⊣⊢ " appears.

Influence quantities and variations for 18S

Influence quantity	Influence range	Measured quantity / measuring range [1]	Variation [2] ± (...% of meas. val. +... digits)
Temperature	- 10 °C...+ 21 °C and +25 °C... + 40 °C	V ⎓	0.05 + 3
		V ~, V ⎓	0.2 + 30
		300 µA / 3 mA	0.2 + 3
		30 mA ⎓	0.1 + 3
		300 mA... 10 A ⎓	0.2 + 3
		300 µA... 300 mA ⎓	0.3 + 30
		3A / 10 A ⎓	0.5 + 30
		300 Ω	0.1 + 5
		3 kΩ... 3 MΩ	0.1 + 3
		30 MΩ	0.6 + 3
		30 nF... 3 µF	0.5 + 3
		30 µF	2.0 + 3
		Hz	0.1 + 3
		-200... + 100 °C	0.5 Kelvin + 2 D
		+ 100... + 850 °C	0.5 + 2
Frequency of the measured quantity	15 Hz... < 45 Hz	300 mV ~	1.0 + 20
	65 Hz... < 200 Hz		1.4 + 20
	> 15 Hz...< 30 Hz	3... 300 V~	1.0 + 20
	> 30 Hz... < 45Hz		0.5 + 20
	> 65 Hz... 400 Hz		0.5 + 20
	> 400 Hz... 1 kHz		1.0 + 20
	> 1 k Hz... 20 kHz		2.0 + 20
	15 Hz... < 30 Hz	1000 V ~	1.0 + 20
	30 Hz... < 45 Hz		0.5 + 20
	> 65 Hz... 1 kHz		2.0 + 20
	15 Hz... < 45 Hz	A~	1.0 + 20
	> 65 Hz... 1kHz		1.0 + 20
	Crest factor CF 1 ...3	V ~ [4], A~ [4]	± 1% of rdg.
	Crest factor CF > 3 ...5		± 3 % of rdg.

The permissible crest factor CF of the AC quantity to be measured is a function of the displayed value :

Waveform of the measured quantity [3]

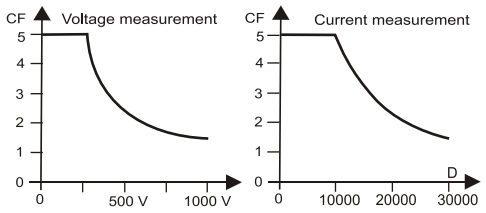

Influence quantity	Influence range	Measured quantity / measuring range	Variation
Battery voltage	⊣⊢ [5] ... < 7.9 V > 8.1 V... 10.0 V	V ⎓	± 6 D
		V ~	± 30 D
		A ⎓	± 30 D
		A~	± (1% of rdg.+ 10D)
		Ω	± 10 D
		3 nF... 30 µF	± 10 D
		Hz	± 6 D
		°C	± 5 D
Relative humidity	75 % 3 days Meter off	V, dB, A, Ω F, Hz °C	1x inherent deviation
DATA		V, dB, A, Ω, Hz	± 20 D
		F	± 2 D
MIN / MAX		V, dB, A, Ω, Hz	± 10 D
		°C, F	± 1 D

1 With zero setting
2 With temperature; Error data is per 10 K change in temperature. With frequency; Error data is valid from a display of 10% of the measuring range.
3 With unknown waveform (crest factor CF > 2), the measurement must be made with manual range selection.
4 Except for sinusoidal waveform
5 From the time the symbol "⊣⊢" appears.

Display

LCD field (65 mm x 30 mm) with analog indication and digital display and with annunciators for unit of measurement, function and various special functions.

Analog

Indication	LCD scale with pointer
Scale length	55 mm on V ⎓ and A ⎓ ; 47 mm on all other ranges
Scaling	+ 5…0…± 30 with 35 scale divisions on ⎓, 0…30 with 30 scale divisions on all other ranges
Polarity indication	With automatic reversal
Overrange indication	By triangle
Sampling rate	20 readings/s, On Ω 10 readings/s

Digital

Display/ height of numerals	Rish multi 12S… 16S, 7 segment numerals / 15mm Rish multi 18S: 7-segment numerals/12 mm
Number of counts	Rish multi 12S…16S, 3 ¾ digit ⏢ 3100 counts Rish multi 18S: 4 ¾ digit ⏢ 31000 counts
Overange display	"**OL**" is shown
Polarity display	"-" sign is shown, When positive pole to "⊥"
Sampling rate	2 readings/s, On Ω and °C:1 reading/s

Display RISH multi 12S... 16S

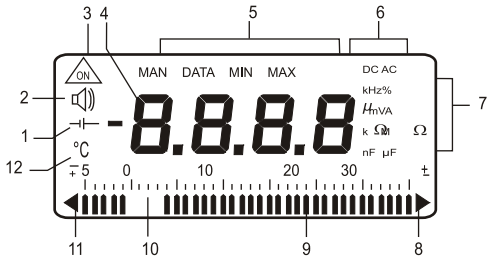

Display RISH multi 18S

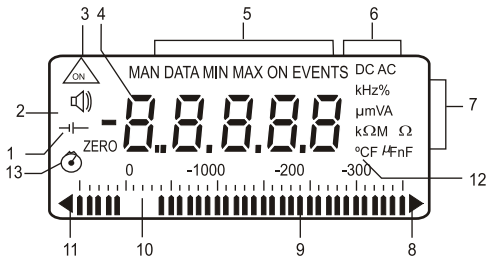

1 Display with low battery voltage
2 Display with sound signal on
3 Symbol for "CONTINUOUSLY ON"
4 Digital display with indication of decimal point and polarity
5 Display with manual range selection as well as with data and MIN/MAX hold
6 Display of the selected function
7 Display of the unit of measurement
8 Display with overrange
9 Pointer for analog indication
10 Scale for analog indication
11 Indication that negative analog range is exceeded
12 Display of the unit 0C when measuring temperature
13 Display with time counter switched on

Applied rules and standards

IEC 61010-1:2001 DIN EN 61010 part 1 VDE 0411 -1	Safety requirements for electrical equipment for measurement, control and laboratory use.
DIN 43751 IS 13875	Digital measuring instruments
EN 61326:2002	Generic emission standard; Residential, commercial and light industry.
EN 61326:2002	Generic immunity standard; residential, commercial and light industry.
VDI/VDE 3540	Reliability of measuring and control equipment.
DIN EN 60529 DIN VDE 0470 part 1	Test equipment and test procedures -Degrees of protection provided by enclosures (IP Code).

Operating controls 12S... 18S

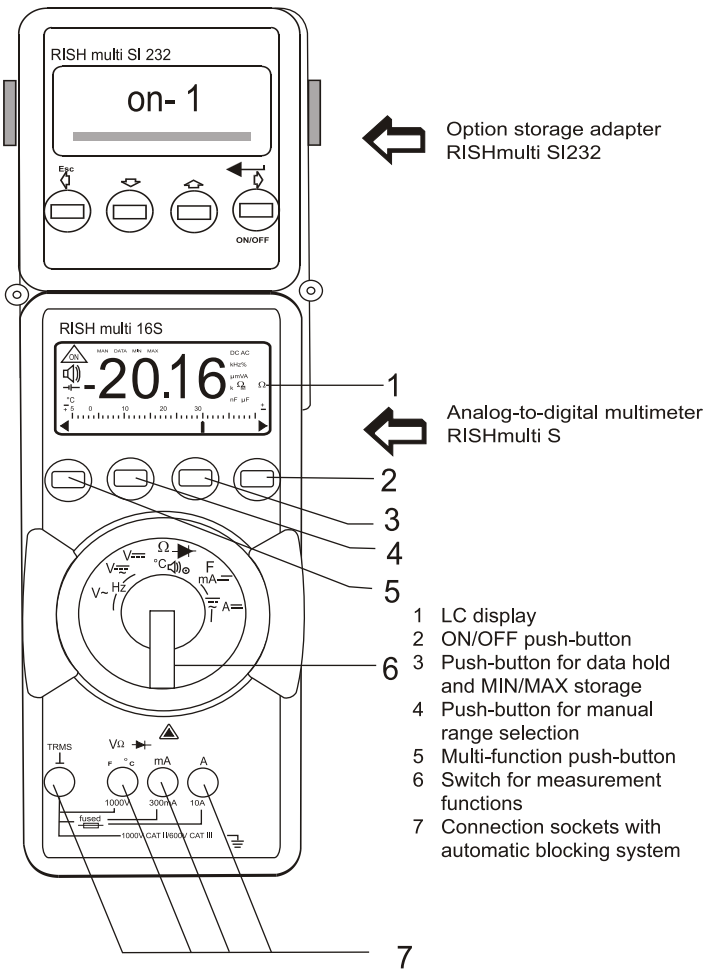

1 LC display
2 ON/OFF push-button
3 Push-button for data hold and MIN/MAX storage
4 Push-button for manual range selection
5 Multi-function push-button
6 Switch for measurement functions
7 Connection sockets with automatic blocking system

Environmental conditions

Working temperature range	RISH multi 12S... 16S -10 °C... + 50 0 C RISH multi 18S -20 °C... + 50 °C
Storage temperature range	-25 °C... + 70 °C (excl. batteries)
Climatic class	RISH multi 12S... 16S 2z/-10/50/70/75% with reference to VDI/VDE 3540 RISH multi 18S, 2z/-20/50/70/75% with reference to VDI/VDE 3540
Altitude above sea level	up to 2000m

Warranty

3 year against defects in materials and workmanship & calibration from the date of purchase.

Mechanical configuration

Protection type	For meters; IP 50, for connection sockets: IP 20
Dimensions	84 mm x 195 mm x 35 mm
Weight	0.35 kg, approx., incl. battery

Scope of delivery

1 multimeter
1 Probe Set
1 copy of operating instructions
1 test certificate
1 rubber holster with tilt stand and carrying strap warranty card

RISHABH

Measure Control Record Analyze Optimize

RISHABH INSTRUMENTS LIMITED
Domestic (India): +91 253 2202099 | marketing@rishabh.co.in
International: +91 253 2202004/06/08/99 | global@rishabh.co.in
www.rishabh.co.in